



www.fine-tek.com


Electromagnetic Flow Meter



FLOW MEASUREMENT FIELD

FineTek is the only inspection institution that owns a Class 2 flow test laboratory in Taiwan. With the most professional R&D and Design Team, it can design and develop high-accuracy electromagnetic flow meters. Moreover, it conducts calibration in Class 1 Flow Laboratory of the National Measurement Laboratory (ITRI Measurement Center), so as to guarantee the flow accuracy on the measurement field.

FineTek's flow laboratory has received certification from the Taiwan Accreditation Foundation and conforms to the regulations of international organizations such as ILAC and APALC. It has the complete ability of uncertainty testing and rating for flow test.

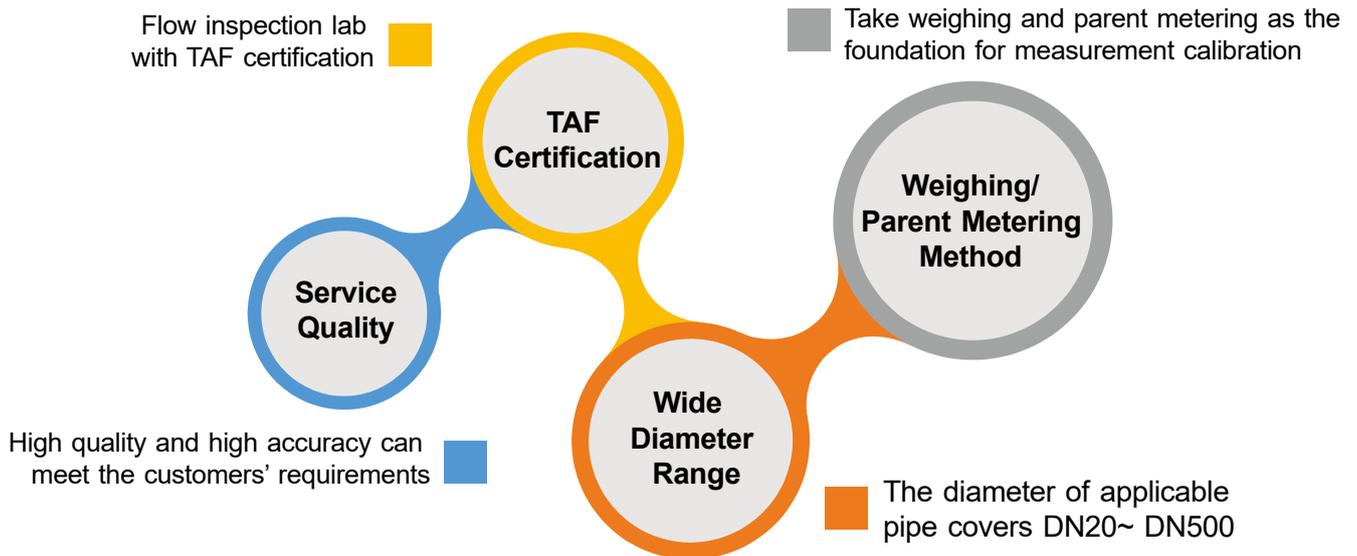

FLOW MEASUREMENT FIELD



PUMP equipment
(The maximum horsepower is 110KW per unit)



Weighing equipment



Control room & Graphical HMI



Piping system I
(Max capacity for four meters calibration simultaneously in above system.)



Piping system II
(Maximum diameter is 500mm)

1. 測試項目 (Testing Item) : 流量試驗
2. 測試日期 (Testing Date) : 2016.05.17
3. 測試地點 (Testing Place) : 室
4. 測試結果 (Result) :
環境溫度 (Environment) :
相對濕度 (Relative Humidity) :


電子秤編號	測試 流量 (m ³ /h)	流速 (m/s)	口徑 (mm)	受測件 (mm ²)	統計分析		
					電子秤量測值	相對偏差 (%)	相對穩定 不穩定度 (%)
3000 kg (8319982827)	254.47	0.88	300	0.6200	0.015	0.625	2.88
				0.6150	0.015	0.260	
				0.6215	0.015	0.215	
3000 kg (8319982827)	127.24	0.50	300	0.8110	0.015	0.811	2.88
				0.80871	0.015	0.80871	
				0.80811	0.015	0.80811	
3000 kg (8319982827)	76.34	0.31	300	0.67009	0.015	0.67009	2.88
				0.65911	0.015	0.65911	
				0.65916	0.015	0.65916	

The exclusive report
(Each flow meter has its own calibration report)

ELECTROMAGNETIC FLOW METER

EPD electromagnetic flow meter is a high-accuracy flow meter manufactured based on the latest international technology. It is widely applied in papermaking, chemical industry, metallurgical industry, drainage, waste water treatment, liquid high-pressure metering, medical care, food, and environmental protection industries.

It is used to measure the non-magnetic liquid and plasma in the enclosed pipe.

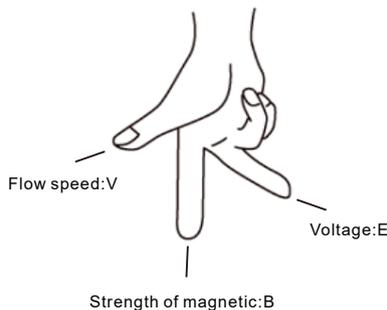


WORKING PRINCIPLE

The working principle of the electromagnetic flow meter is based on the Faraday law of electromagnetic induction. When the conducting liquid flows in the orthogonal direction of the magnetic line direction, it will cut the magnetic lines and generate induced voltage, which shows linear relationship with the flowing speed. Thus, the fluidic volume flow can be calculated.

EPD electromagnetic flow meter is mainly composed of the sensor and transmitter. The measuring tube of the sensor is equipped with the excitation coils upward and downward. The transmitter supplies the excitation current, which generates the magnetic field which goes through the measuring tube once it is powered on. A pair of induction electrodes installed on the inner side of the measuring tube comes in contact with the liquid to guide the induced voltage to the sensor.

APPLICATIONS

- Waste water treatment
- Tapped water purification
- Sewerage
- Sea water desalination module
- Dyeing machines
- Solar energy and PCB wet processing
- Food manufacturing
- Pharmaceutical machines

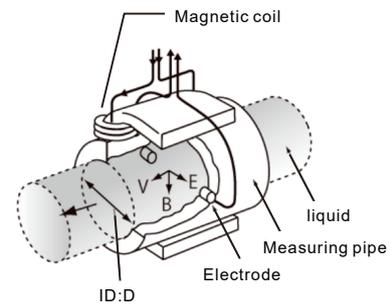

FEATURES

Low impact on environmental matter

- The measurement results are not affected by the change in liquid density, viscosity, temperature, pressure and conductivity.
- It can be widely applied in the conducting liquids that may contain fiber, solid granules and suspended matters.
- Enclosure protection rating: IP67/NEMA 4X

Wide measurement range & high efficiency

- The wide measurement turndown ratio can be reach 1:100, which can be set randomly and achieve high accuracy for small flow measurement.
- Highly-integrated backlit display of two rows, dual isolation, parameter setting, menu-type operation, memory function, reliable programming, password lock and access, small signal elimination, non-linear correction and two-way measurement.
Various outputs: Current output 4~20mA,
- frequency output 2~8KHz and RS485 communication.

Multiple self-diagnosis function

- Power-saving and low fault rate: The measuring tube is without baffle and movable parts, so it won't cause pressure loss and jam.
- Smart self-detection and self-diagnosis function, as well as various alarms

The low installation cost

- It is easy-to-install with low requirements for the straight tube section (Front 5D and rear 2D)

IECEx ,CSA Explosion proof(EPD30)

Available for records for parameter modifications, boot/ shut down device(Option)

Authority management is available in menu (Option)

SPECIFICATION

Item	EPD36 Standard type
Display	LCM 128*64 pixel backlit type
Buttons	Tri-button operation
Communication interface	RS-485 (Modbus) (Optional support for ZigBee Pro wireless transmission)
Accuracy	±0.5% of reading@1m/s(0.2% optional)
Medium temperature	-20 ~ 150°C(PFA Lining)
Ambient temperature	-40 ~ 70 °C*
Fluidic conductivity	> 5 uS/cm
Measuring scope	0.1m/s ~ 10m/s
Current output accuracy	0.1% of Pulse Output Accuracy Temperature coefficient (100 ppm/°C)
Operating pressure	10 Kg/cm ²
Current output mode	Proactive
Analog output	4 ~ 20 mA
Maximum load of current output	< 700W
Alarming current	3.6mA or 22 mA
Frequency output scope	2 ~ 8 KHz
Pulse width	Automatic (pulse width 50%)
Pulse mode	Isolated NPN Transistor output 32vdc/200mA
Time constant	1~100 s
Control output (DO)	Isolated NPN Transistor output 32vdc/200mA; 2-CH
Control input (DI)	Dry contact ON < 200W ; 1,000W < OFF ; 1-CH
Data logger(Optional)	500 items. With calendar (Internal battery: Lift time > 6 month)
Baud rate	1200 ~ 57600 bps
Protection rating	IP67 / NEMA 4X
Enclosure material	Aluminum alloy
Input power	DC 24V
Power consumption	< 10W
Wire inlet specification	1/2" NPT
Excitation mode	Pulse DC
Vibration regulation	MIL-STD-202G-201A:2002
EMC regulation	IEC/EN 61326-1 Class A table2

*It can't display when LCM is lower than -20°C.

MATERIAL SELECTION


※Electrode material

Electrode material	Anti-corrosion property
Stainless steel (316L)	It is applied in water, sewage and organic and non-organic corrosive medium.

※Lining material

Lining material	Main properties	Application scope
PFA	<ol style="list-style-type: none">1. Stable chemical properties, resistant to various acid, alkane, and salt solutions and various organic solvents. It is not tolerant to the corrosion of ClF₃, high-temperature OF₃ and high-speed liquid oxygen and ozone.2. The anti-abrasion property is average.	<ol style="list-style-type: none">1. -20~150°C2. Strong corrosive medium such as concentrated acid and alkane.

APPEARANCE AND DIMENSION AND FLANGE CONNECTION DIMENSION STANDARD TYPE

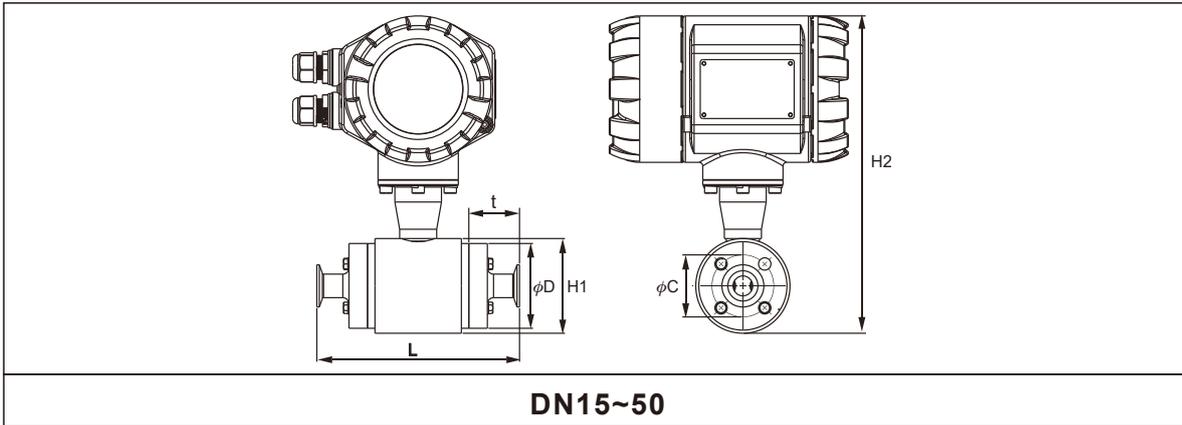

Connection specification		Tri-Clamp			
Nominal diameter(mm)		15	25	40	50
Lining material		PFA			
Length	L	164	164	258.6	258.6
External diameter	ϕD	68.3	81.1	106.3	106.3
PCD	ϕC	50	60	83	83
Flange thickness	t	41	41	61.5	61.5
Quantity of screw holes	N	4	4	4	4
Height of sensor casing	H1	76.3	89.1	114.3	114.3
Total height	H2	256	270	294	294
Weight(kg)	H1	4.9	5.7	8.6	9.1

Connection specification

Tri-Clamp	DN	d_i (mm)	G (mm)
	15	15.8	25
	25	22.1	50.5
	40	34.8	50.5
	50	47.5	64


PIPE DIAMETER, FLOW RANGE AND ACCURACY SELECTION

Pipe diameter (mm)	Flow range (m ³ /h)	
	Flowing speed 0.1~1.0m/s	Flowing speed 1.0~10m/s
15	0.06~0.64	0.64~6.4
25	0.17~1.77	1.77~17.7
40	0.45~4.5	4.5~45.2
50	0.71~7.1	7.1~71



INSTALLATION INSTRUCTIONS


1. The flow meter must be free from strong electromagnetic field. The magnetic intensity of the flow meter installation site must be smaller than 400A/m (It should not be installed near large motors or transformers).
2. It should be installed at the lower point and the vertically upward point of the horizontal pipe. Don't install it at the highest point and the vertically downward point of the pipe.

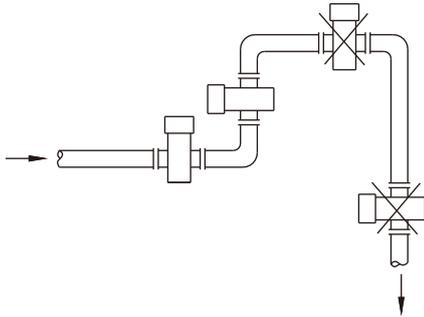


3. It should be installed at the rising point of the pipe.




4. It should be installed at the lower point of the pipe when it is installed on the pipe with opening for drainage.




5. If the pipe gap exceeds 5m, the air release valve should be installed at the downstream of the sensor. The downstream of the sensor should have some back pressure.

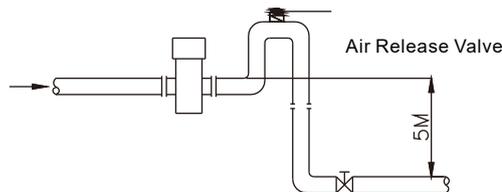

6. The control valve and cut valve should be installed at the downstream of the sensor rather than the upstream.

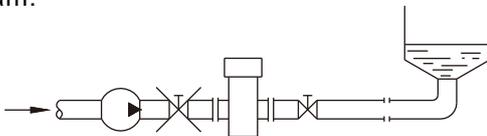


7. The sensor should be installed at the pump outlet rather than the inlet.



8. The fluidic must flow towards the arrow direction of the flow meter.
9. The axial line of the measuring electrode must be approximate to the horizontal direction (The angle of from the horizontal direction).
10. The measuring pipe must be completely filled with liquid.


INSTALLATION INSTRUCTIONS

11. The straight tube section is required to be at least 5D (internal diameter of the flow meter) on the front side, and at least 2D on the rear side.



12. When measuring the mixture of different media, the distance between the mixing point and the flow meter must be 30D at least.


13. For convenient cleaning and maintenance of the flow meter, a bypass pipe must be installed.

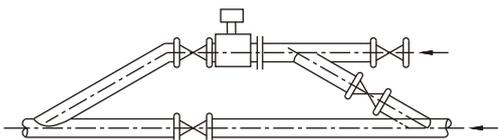


14. When installing the sensor, it should ensure that the measuring pipe and the process pipe must be on the same axial line. For the flow meter with the pipe meter of 50mm or below, the axial line deviation should not exceed 2mm. For those of DN65□DN150, the axial line deviation should not exceed 3mm. For those of \geq DN200, the axial line deviation should not exceed 4mm.

15. The shim installed between the flanges should have excellent anti-corrosion property. The shim should not intrude in the pipe, which will affect the fluidic in the pipe.


16. The sensor and transmitter should be equipped with high-quality independent grounding wire (The section area of the copper core is 1.6mm²). The grounding resistance should be $<10\Omega$. If the grounding is poor, it won't work normally. The grounding ring is needed if the pipe connecting with the sensor is insulating, and the material of the grounding ring should be the same as that of the electrode. If the test medium is abrasive, the neck grounding ring should be selected.

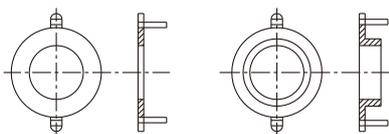


16.1 It is for installing the flow meter on the metal pipe not coated with insulating layer internally.



16.2 When installing the flow meter on the protective pipe of the cathode, the pipe with the protection of electrolytic corrosion generally has insulating walls and protruding sides. Thus, during installation, the grounding ring and the flanges on the pipe should be insulating.



16. When installing the flow meter on the plastic pipe or the pipe with insulating coating material, paints or lining, grounding rings on both ends of the sensor should be installed.



MODEL NUMBER / ORDER CODE COMPARISON TABLE

ORDERING INFORMATION

Model Number	Order Code
EPD36	EPD10300-A

EPD1 0 3 0 0 -A ^⑩ ^⑪ ^⑫ I 0 0 MC 1 4 MC A D F 0 0 0 0

⑩ ⑪ ⑫ Pipe diameter

015: 15mm
025: 25mm
040: 40mm
050: 50mm

⑬ ⑭ ⑮ Connection specification

I 00: Tri-clamp

⑯ ⑰ Connection material

MC: SUS316L

⑱ ⑲ Lining material

14: PFA

⑳ ㉑ Electrode material

MC: SUS316L

㉓ Power suppl

D: 24Vdc

㉔ Accuracy

F: 0.5%

SETTING VALUES

Main Menu	Sub Menu	Unit	Default	Setting Range
Fast Set(0)	Device Tag Num (1.1)			
	Zero Adj. (2.1)			
	Flow Span (1.5)			
	Flow Unit (1.4)			
	Low cutoff (2.4)			
	Damping Time (3.1)			
	Pulse Out Unit (3.3)			
	Total Reset (1.9)			

The parameter is linking form standard manu

Main Menu	Sub Menu	Unit	Default	Setting Range
Basic Set (1)	Device Tag Num (1.1)		00001	00001~65535
	Measure Type (1.2)	-	Water	Water
	Tube Size (1.3)	mm	actual	10,15,25,32,40,50,65,80,100 125,150,200,250,300,350,400,450,500
	Flow Unit (1.4)	-	m ³ /h	L/(s,min,h), m ³ /(s,min,h), gal/(s,min,h), kg(s,min,h), Ton(s,min,h) (Flow rate* Liquid density = weight) "L/s", "L/m", "L/h", "m3/s", "m3/m", "m3/h", "gal/s", "gal/m", "gal/h", "kg/s", "kg/m", "kg/h", "Ton/s", "Ton/m", "Ton/h", "m3/d"
	Flow Span (1.5)	=Flow Rate Unit	$(5m/s) \times (Diameter/2)^2 \times \pi \times \text{Unit of Flow Forward}$	$(0.1 \sim 10.0m/s) \times (Diametermm/2)^2 \times \pi \times \text{Unit of Flow Forward}$
	Direction (1.6)	dir	Forward	Forward,Reverse
	Total Unit (1.7)	-	m ³	Liter,gal,m ³ ,kg,Ton
	Total Mode (1.8)	none	Forward	Forward,Reverse,Bi-direction
	Total Reset (1.9)	none	Cancel	Cancel,Accept

Main Menu	Sub Menu	Unit	Default	Setting Range
Advanced Set (2)	Zero Adj. (2.1)	m/s	actual	-0.5000~+0.5000
	K-Factor (2.2)	none	1.000	0.000~3.000
	Density (2.3)	g/cm ³	1.0000	0.0001~9.9999
	Low cutoff (2.4)	%	0.5	0.00~100.00
	Fwd. Init. (2.5)	=Total Unit	0	0~9999999999
	Rev. Init.(2.6)	=Total Unit	0	0~9999999999

SETTING VALUES

Main Menu	Sub Menu	Unit	Default	Setting Range
I/O Signal Set (3)	Damping Time (3.1)	second (s)	3	0~100
	Pulse Out Mode (3.2)	none	Pulse NO	Pulse NO, Pulse NC, Frequency
	Pulse Out Unit (3.3)	Unit/pulse	0.1 L	0.001~100(L,gal,m ³ ,g,kg,Ton) m ³ /pulse,gal/pulse,m ³ /pulse g/pulse,kg/pulse,Ton/pulse
	Max. Freq. (3.4)	Hz,kHz	2K	1~8K (00.0000)
	Curr. Mode (3.5)	none	4-20	4-20,0-20
	4mA Fine-Tune (3.6)	count	0	-5000~5000
	20mA Fine-Tune (3.7)	count	0	-5000~5000
	Input1 Func. (3.8)	N/A	None	None, Total Reset
	Input1 Type (3.9)	N/A	NO	NO,NC
	Filter Variation (3.10)	m/s	1	0.000~10.000
	Filter Weight (3.11)	%	10	0~100
	Median Filter(3.12)	%	Enable	Disable,Enable

Main Menu	Sub Menu	Unit	Default	Setting Range
Alarm Set (4)	Max. Flow (4.1)	Flow Rate Unit	Max.	Max. Flow Rate
	Min. Flow (4.2)	Flow Rate Unit	Min.	Min. Flow Rate
	Empty Tube Set (4.3)	N/A	Enable	Enable, Disable
	Output 1 Func. (4.4)	N/A	Max. Flow Rate	Max. Flow Rate, Min. Flow Rate, Empty Tube, System Alarm
	Output 1 Type (4.5)	N/A	No	NO,NC
	Output 2 Func. (4.6)	N/A	Min. Flow Rate	Max. Flow Rate, Min. Flow Rate, Empty Tube, System Alarm
	Output 2 Type (4.7)	N/A	No	NO,NC
	Curr. Func. (4.8)	N/A	None	Empty Tube, System Alarm
	Alarm Curr. (4.9)	mA	3.6	3.6,3.8,20.5,22
	Temp. Alarm. (4.10)	N/A	1	0:OFF, 1:ON

SETTING VALUES

Main Menu	Sub Menu	Unit	Default	Setting Range	
System Set (5)	Language (5.1)	N/A	English	English, Traditional Chinese, Simplified Chinese	
	System Info.(5.2)	Tube Status	N/A	Actual	(Normal, Empty)
		Act. Flow Speed	m/s	Actual	N/A
		Resistance	kΩ	Actual	N/A
		Status Code	N/A	Actual	0000 0000 ~ FFFF FFFF
	Self-Test (5.3)	N/A	/A	Cancel	Normal, Circuit Fail, Excitation Fail, Amb. Temp, Electrode Coating
	Analogy Input (5.4)	4mA Display	N/A	0000	0~9999
		20mA Display.	N/A	1000	0~9999
		4-20mA Unit	N/A	Kpa	None, Kpa, Mpa, Psi, Bar, °C, °F
		Dot	N/A	1	0~3
	ModBus Comm. (5.5)	Modbus ID(2.13.1)	/A		~255
		BaudRate(2.13.2)	S		1200,2400,4800,9600,19200 38400,57600
		Data bit(2.13.3)	N/A	8	8
		Parity(2.13.4)	N/A	none	none, odd, even
		Stop bit(2.13.5)	/A		1,2
Recovery Default (5.6)	N/A	N/A	Cancel	Cancel, Accept	
Mains Frequency (5.7)	N/A	Hz	50	50, 60	
LCM Contrast Brightness(5.8)	N/A	%	50	10~100	
Manu Password (5.9)	User Password(5.9.1)	N/A	00000	0~99999	
	Admin Password(5.9.2)	N/A	00000	0~99999	

Main Menu	Sub Menu	Unit	Default	Setting Range
Simulation (6)	Flow Speed (6.1)	m/s	0	-10 ~ 10
	Flow Rate (6.2)	Flow Rate Unit	0	0~max.
	Output Curr. (6.3)	mA	4mA	3.6~22
	Output Freq. (6.4)	Hz(pulse/sec)	2	8000
	Output1 Status (6.5)	N/A	OFF	ON/OFF
	Output2 Status (6.6)	N/A	OFF	ON/OFF
	Input1 Status (6.7)	N/A	Actual	ON/OFF
	Input Curr. (6.8)	N/A	Actual	0~24mA

Main Menu	Sub Menu	Unit	Default	Setting Range
System Log (7)	Date Set (7.1)	N/A	actual	year : 17~99, month : 01~12, day : 01~31
	Time Set (7.2)	N/A	actual	hour : 00~23, minute : 00~59, sec : 00~59
	Log data clear (7.3)	N/A	Cancel	Cancel, Accept
	System Log Info (7.4)	N/A	actual	N/A

Main Menu	Sub Menu	Unit	Default	Setting Range
Infomation (8)	F.W. Version(8.1)		actual	

※Sub menu 1.3、1.9、2.2、2.5、2.6、.6、5.9、7.3, only the admin can change.

APPLICATION DEMO



Pharmaceutical



Pharmacy



Beverage



Electronics



Food & Beverage



Incinerator



Mining



Plastic

TUCHENG PLANT/YILAN PLANT



EPD APPLICATION / ORDER FORM

Company Profile

Company Name: _____ Contact Person: _____
E-mail: _____ Phone: _____ Tax: _____

Application

Medium: _____ Temperature: _____ Sanitary Degree Request: Yes NO
Conductivity: _____ Viscosity: _____
Diameter of Tube (DN) : _____ Accuracy Request(%): _____ Ambient Temp.: _____
Normal Flow Rate(m³/h): _____ Max. Flow Rate(m³/h): _____ Min. Flow Rate(m³/h): _____
Connection Spec: _____ Connection Material**: _____
Pressure (Kg/cm²): _____ Max. Static Pressure (Kg/cm²): _____ **SUS304, SUS316, SUS316L
Lining Material*: _____ Electrode Material***: _____

*PTFE、NBR、Neoprene

***SUS316L, Hastelloy Alloy, Titanium, tantalum

Power: 110Vac 220Vac 24Vdc
Output: 4-20mA/Pulse(freq) RS-485/Modbus
Grounding: NO YES
Installation Direction: Horizontal Vertical
Vibration Inside Tube: NO YES
Strong Magnetic Nearby: NO YES
Explosion Proof: NO YES
Explosion Proof Code: _____



■ Head Quarter

- Taiwan
 FineTek Co., Ltd. - Taipei Head Quarter
 No.16, Tzuchiang St., Tucheng Industrial Park
 New Taipei City 236, Taiwan
 TEL: 886-2-2269-6789
 FAX: 886-2-2268-6682
 EMAIL: info@fine-tek.com

■ North America

- California, U.S.
 Aplus Finetek Sensor Inc. - US Office
 355 S. Lemon Ave, Suite D
 Walnut, CA 91789
 TEL: 1 909 598 2488
 FAX: 1 909 598 3188
 EMAIL: info@aplusfine.com

■ Europe

- Germany
 FineTek GmbH - Germany Office
 Bei den Kämpen 26
 21220 Seevetal-Ramelsloh, Germany
 TEL: +49-(0)4185-8083-12
 FAX: +49-(0)4185-8083-80
 EMAIL: info@fine-tek.de

■ Asia

- China
 Fine automation Co., Ltd. - Shanghai Factory
 No.451 DuHui Rd, MinHang District, Shanghai,
 China 201109
 TEL: 86-21-6490-7260
 EMAIL: info.sh@fine-tek.com

- Singapore
 FineTek Pte Ltd. - Singapore Office
 37 Kaki Bukit Place, Level 4 Singapore 416215
 TEL: 65-6452-6340
 EMAIL: info.sg@fine-tek.com

- Indonesia
 PT. FineTek Automation Indonesia - Indonesia Office
 PERGUDANGAN TUNAS BITUNG
 JL. Raya Serang KM. 13,8, Blok C3 No. 12&15,
 Bitung Cikupa, Tangerang 15710
 TEL: 62 (021)-2958-1688
 EMAIL: info.id@fine-tek.com

- Mütec Instruments GmbH - Germany Office
 Bei den Kämpen 26
 21220 Seevetal-Ramelsloh, Germany
 TEL: +49-(0)4185-8083-0
 FAX: +49-(0)4185-8083-80
 EMAIL: muetec@muetec.de



Distributor: